

Automated Epilepsy Diagnosis Using Interictal Scalp EEG

Forrest Sheng Bao, Jue-Ming Gao, Jing Hu, Donald Y.-C. Lie, Yuanlin Zhang and K. J. Oommen

Abstract—Approximately over 50 million people worldwide suffer from epilepsy. Traditional diagnosis of epilepsy relies on tedious visual screening by highly trained clinicians from lengthy EEG recording that contains the presence of seizure (ictal) activities. Nowadays, there are many automatic systems that can recognize seizure-related EEG signals to help the diagnosis. However, it is very costly and inconvenient to obtain long-term EEG data with seizure activities, especially in areas short of medical resources. We demonstrate in this paper that we can use the interictal scalp EEG data, which is much easier to collect than the ictal data, to automatically diagnose whether a person is epileptic. In our automated EEG recognition system, we extract three classes of features from the EEG data and build Probabilistic Neural Networks (PNNs) fed with these features. We optimize the feature extraction parameters and combine these PNNs through a voting mechanism. As a result, our system achieves an impressive 94.07% accuracy, which is very close to reported human recognition accuracy by experienced medical professionals.

I. INTRODUCTION

EPILEPSY is the second most common neurological disorder, affecting 1% of world population [1]. Eighty-five percent of patients with epilepsy live in the developing countries [2]. Electroencephalogram (EEG) is routinely used clinically to diagnose epilepsy [3]. Long-term video-EEG monitoring can provide 90% positive diagnostic information [4] and it has become the golden standard in epilepsy diagnosis. For the purpose of this research, we define the term “the diagnosis of epilepsy” as the determination of whether a person is epileptic or non-epileptic [5].

Traditional diagnostic methods rely on experts to visually inspect lengthy EEG recordings, which is time consuming and problematic due to the lack of clear differences in EEG activity between epileptic and non-epileptic seizures [6], particularly in seizures of frontal origin. Many automated seizure recognition techniques, therefore, have emerged [6]–[17]. The approach of using automatic seizure recognition/detection algorithms would still require the recording of clinical seizures. Therefore, very long continuous EEG recording, preferably with synchronized video for several days or weeks, are needed to capture the seizures. The long-term EEG recording can greatly

disturb patients’ daily lives. Another clinical concern is that very unfortunately, 50-75% of epilepsy patients in the world reside in areas which lack the medical resources and trained clinicians, that are needed to make such a process feasible [2]. Consequently, an automated EEG epilepsy diagnostic system would be very valuable if it does not require data containing seizure activities (i.e., ictal) to arrive at the diagnosis. However, to the authors’ best knowledge, we are not aware of any report on automated epilepsy diagnostic system using only interictal scalp EEG data.

Previous research has also attempted at creating automated epilepsy diagnostic systems using interictal EEG data [13], [18]. However, in those trials, only *intracranial* EEG data from patients are used, and the EEG artifacts have been carefully removed manually. It is very expensive to obtain intracranial EEG recordings that are relatively artifact free for every epilepsy patient, which is especially impractical in poor and rural areas. Therefore, we have built an automated epilepsy diagnostic system with very good accuracy that can work with scalp EEG data that contain noise and artifacts.

Artificial Neural Network (ANN) has been used for seizure-related EEG recognition [10]–[15]. We use in this work one kind of ANN as the classifier, namely the Probabilistic Neural Network (PNN), for its high speed, high accuracy and real-time property in updating network structure [19]. It is very difficult to directly use raw EEG data as the input of an ANN [20]. Therefore, the key is to parameterize the EEG data into features prior to the input into the ANN. We use features that are used in previous studies on seizure-related EEG, namely, the power spectral feature, fractal dimensions and Hjorth parameters. A simple classifier voting scheme [21] and parameter optimization are used to improve the accuracy.

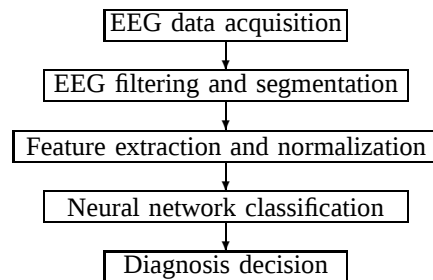


Fig. 1. Flow diagram of our EEG classification scheme

This research is supported by the Fall 2007 Research Enrichment Fund Grant of Texas Tech University. Human subject data used in this research has been approved and are already exempt by Protection of Human Subjects Committee IRB committee of Texas Tech University under “501209 Diagnosis, Monitoring, Seizures Prediction and Intervention for Epilepsy Patients Using an Intelligent Scalp-EEG Signal Analysis System.”

F. S. Bao, D. Y.-C. Lie and Y. Zhang are with Dept. of Computer Science and Dept. of Electrical & Computer Engineering, Texas Tech University, Lubbock 79409 Texas, USA forrest.bao@gmail.com

J. Hu and J.-M. Gao are with Dept. of Neurosurgery, Jiangsu Provincial Hospital of Chinese Medicine, Nanjing, Jiangsu China

K. J. Oommen is with Dept. of Neurology, Texas Tech University Health Sciences Center, Lubbock 79409 Texas, USA

The final accuracy of our system on distinguishing interictal scalp EEG of epileptic patients vs. the scalp EEG of healthy people is 94.07%, which is very close to currently reported human diagnosis accuracy [22].

II. DATA ACQUISITION

We compose a data set based on 22-channel routine scalp EEG recordings from Dept. of Neurology, Jiangsu Provincial Hospital of Chinese Medicine, China. The data is from 6 normal people and 6 epileptic patients (in interictal period only). It is recorded at 200 Hz sampling rate using the standard international 10-20 system with referential montage. Whereas other research [13] EEG recordings are cut into segments of 4096 (i.e., 2^{12}), our complete data set has 22,353 segments per channel, and 491,766 segments in total.

III. FEATURE EXTRACTION

Three classes of features are extracted to characterize EEG signal: Power Spectral Features, describing its energy distribution in the frequency domain, Fractal Dimensions outlining its fractal property, and Hjorth Parameters, modeling its chaotic behavior.

A. Power Spectral Features

As one can see from Fig. 2, power spectrum is a good way to distinguish different kinds of EEG signals.

To a time series $x_1, x_2, \dots, x_N$, its Fast Fourier Transform (FFT) $X_1, X_2, \dots, X_N$ is estimated as

$$X_k = \sum_{n=1}^N x_n W_N^{kn}, \quad k = 1, 2, \dots, N$$

, where $W_N^{kn} = e^{-\frac{j2\pi kn}{N}}$ and N is the series length.

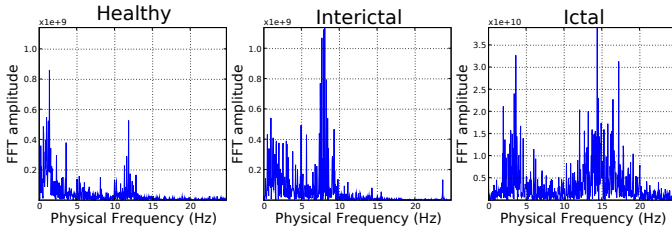


Fig. 2. Typical FFT results of 3 EEG segments (Raw data in μV)

Based on the FFT result, Power Spectral Intensity (PSI) of each f_{step} Hz bin in a given band $f_{\text{low}} - f_{\text{up}}$ Hz is evaluated as

$$PSI_k = \sum_{i=\lfloor N \frac{f_{\min}}{f_s} \rfloor}^{\lfloor N \frac{f_{\max}}{f_s} \rfloor} X_i, \quad k = 1, 2, \dots, K \quad (1)$$

, where $f_{\min} = 2k$, $f_{\max} = 2k + 2$, $K = (f_{\text{up}} - f_{\text{low}}) / f_{\text{step}}$, f_s is the sampling rate and N is the series length. $f_{\min}$ and $f_{\max}$ are the lower and upper boundaries of each bin, respectively.

We use Relative Intensity Ratio (RIR) as the Power Spectral Features. It is defined as

$$RIR_j = \frac{PSI_j}{\sum_{k=1}^K PSI_k}, \quad j = 1, 2, \dots, (f_{\text{up}} - f_{\text{low}}) / f_{\text{step}}.$$

B. Petrosian Fractal Dimension (PFD)

PFD is defined as:

$$PFD = \frac{\log_{10} N}{\log_{10} N + \log_{10} \left(\frac{N}{n + 0.4N_\delta} \right)}$$

, where N is the series length and N_δ is the number of sign changes in the signal derivative [23].

C. Higuchi Fractal Dimension (HFD)

Higuchi's algorithm [24] constructs k new series from the original series $x_1, x_2, \dots, x_N$ by

$$x_m, x_{m+k}, x_{m+2k}, \dots, x_{m+\lfloor \frac{N-m}{k} \rfloor k} \quad (2)$$

, where $m = 1, 2, \dots, k$.

For each time series constructed from (2), the length $L(m, k)$ is computed by

$$L(m, k) = \frac{\sum_{i=2}^{\lfloor \frac{N-m}{k} \rfloor} |x_{m+ik} - x_{m+(i-1)k}| (N-1)}{\lfloor \frac{N-m}{k} \rfloor k}$$

The average length $L(k)$ is computed as

$$L(k) = \frac{\sum_{i=1}^k L(i, k)}{k}$$

This procedure repeats $k_{\max}$ times for each k from 1 to $k_{\max}$, and then uses a least-square method to determine the slope of the line that best fits the curve of $\ln(L(k))$ versus $\ln(1/k)$. The slope is the Higuchi Fractal Dimension. In this paper, $k_{\max} = 5$.

D. Hjorth Parameters

To a time series $x_1, x_2, \dots, x_N$, the Hjorth mobility and complexity [25] are respectively defined as

$$\sqrt{\frac{M2}{TP}} \text{ and } \sqrt{\frac{M4 \cdot TP}{M2 \cdot M2}}$$

, where $TP = \sum x_i / N$, $M2 = \sum d_i / N$, $M4 = \sum (d_i - d_{i-1})^2 / N$ and $d_i = x_i - x_{i-1}$.

IV. PROBABILISTIC NEURAL NETWORK

In machine learning, a classifier is essentially a mapping from the feature space to the class space. An Artificial Neural Network (ANN) implements such a mapping by using a group of interconnected artificial neurons simulating human brain. An ANN can be trained to achieve expected classification results against the input and output information stream, such that there is not a need to provide a specified classification algorithm.

PNN is one kind of distance-based ANNs, using a bell-shape activation function. Compared with traditional back-propagation (BP) neural network, PNN is considered more suitable to medical application since it uses Bayesian strategy, a process familiar to medical decision makers [26]. Decision boundaries of PNN can be modified in real-time as new data becomes available [19]. There is no need to train the network over the entire data set again. We can therefore quickly update our network as more and more patients' data becomes available.

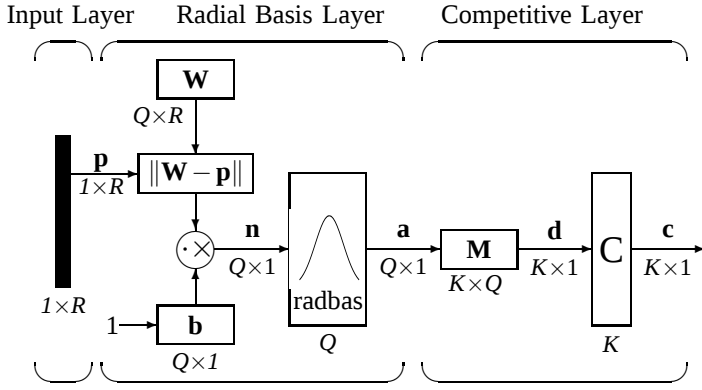


Fig. 3. PNN structure, R: number of features, Q: number of training samples, K: number of classes. The input vector $\mathbf{p}$ is presented as a black vertical bar.

Our PNN has three layers: the Input Layer, the Radial Basis Layer which evaluates distances between input vector and rows in weight matrix, and the Competitive Layer which determines the class with maximum probability to be correct. The network structure is illustrated in Fig. 3. Dimensions of matrices are marked under their names.

A. Radial Basis Layer

In Radial Basis Layer, the vector distances between input vector $\mathbf{p}$ and the weight vector made of each row of weight matrix $\mathbf{W}$ are calculated. Here, the vector distance is defined as the dot product between two vectors [19]. The dot product between $\mathbf{p}$ and the i -th row of $\mathbf{W}$ produces the i -th element of the distance vector matrix, denoted as $\|\mathbf{W} - \mathbf{p}\|$. The bias vector $\mathbf{b}$ is then combined with $\|\mathbf{W} - \mathbf{p}\|$ by an element-by-element multiplication, represented as “ $\cdot \times$ ” in Fig. 3. The result is denoted as $\mathbf{n} = \|\mathbf{W} - \mathbf{p}\| \cdot \mathbf{b}$.

The transfer function in PNN has built into a distance criterion with respect to a center. In this paper, we define it as

$$\text{radbas}(n) = e^{-n^2} \quad (3)$$

Each element of $\mathbf{n}$ is substituted into (3) and produces corresponding element of $\mathbf{a}$, the output vector of Radial Basis Layer. We can represent the i -th element of $\mathbf{a}$ as

$$\mathbf{a}_i = \text{radbas}(\|\mathbf{W}_i - \mathbf{p}\| \cdot \mathbf{b}_i) \quad (4)$$

, where $\mathbf{W}_i$ is the i -th row of $\mathbf{W}$ and $\mathbf{b}_i$ is the i -th element of bias vector $\mathbf{b}$.

1) *Radial Basis Layer Weights*: Each row of $\mathbf{W}$ is the feature vector of one training sample. The number of rows equals to the number of training samples.

2) *Radial Basis Layer Biases*: All biases in radial basis layer are set to $\sqrt{\ln 0.5/s}$ resulting in radial basis functions that cross 0.5 at weighted inputs of $\pm s$, where s is the spread constant of PNN. According to our experience, $s = 0.1$ can result in the highest accuracy.

B. Competitive Layer

There is no bias in Competitive Layer. In this layer, the vector $\mathbf{a}$ is first multiplied by layer weight matrix $\mathbf{M}$, producing an output vector $\mathbf{d}$. The competitive function $\mathbf{C}$ produces a 1

corresponding to the largest element of $\mathbf{d}$, and 0's elsewhere. The index of the 1 is the class of the EEG segment. $\mathbf{M}$ is set to $K \times Q$ matrix of Q target class vectors. If the i -th sample in training set is of class j , then we have a 1 on the j -th row of i -th column of $\mathbf{M}$.

V. COMBINING CLASSIFIERS USING VOTING

A simple voting scheme [21] is used to improve the classification accuracy in this paper. We first build one component classifier for each channel and then combine them as follows. Given 22 segments collected at the same time (from different channels), each of them will be classified by the component classifier for the same channel. The component classifier of each channel will judge whether the given EEG segment is epileptic. The final classification decision is based on the vote of each component classifier. The voting rule we use here is the majority rule. Fig. 4 shows the diagram on how the combined classifiers work.

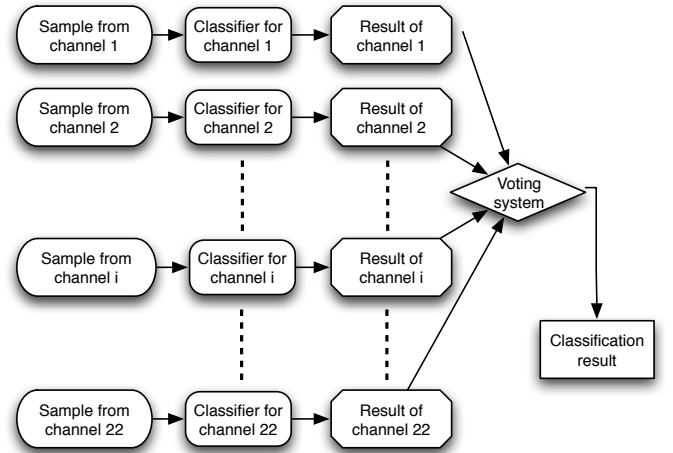


Fig. 4. Classification Voting Scheme

VI. EXPERIMENTAL RESULTS

In the experiments, we use MATLAB Neural Network Toolbox to implement PNN. The data used in the experiments is labeled as interictal (positive) or healthy (negative). The interictal data set has the same size as the healthy one. The testing method for PNN is Leave-One-Out Cross-Validation (LOOCV) [21], where exactly one sample is used as the test sample while all the rest as training samples and such process repeats until every sample has been used as a test sample for exactly once.

We notice that different parameters used in feature extraction can lead to different classifier performance. We will show the experimental results using default feature extraction parameters in the first section while using optimized parameters in the second section.

TABLE I
SINGLE CHANNEL CLASSIFICATION ACCURACY USING PNN

channel	RIRs, FDs & Hjorth's	FDs & Hjorth's	FDs	RIRs	Hjorth's	RIRs & FDs	RIRs & Hjorth's
Fp1	76	63	58	72	63	75	73
Fp2	78	62	58	73	54	77	74
F3	75	61	56	71	59	73	73
F4	80	64	59	76	62	79	77
C3	81	67	62	77	58	80	78
C4	77	63	58	73	59	76	74
P3	76	62	55	73	57	75	74
P4	81	64	60	77	59	80	78
O1	79	62	55	76	58	78	76
O2	81	61	56	75	56	78	79
F7	80	66	57	76	63	79	78
F8	85	70	57	81	61	82	84
T3	81	67	66	76	59	78	79
T4	81	62	60	78	53	80	79
T5	79	67	59	72	59	75	77
T6	78	67	57	70	62	74	75
A1	80	66	58	72	61	77	77
A2	80	61	56	72	60	76	75
Fz	81	65	59	78	54	80	79
Pz	79	65	57	73	56	77	75
Cz	81	66	62	77	56	80	78
Oz	82	61	59	77	54	80	79

A. Classification using default feature extraction parameters

The features are extracted using the default parameters described in Sec. II. We have carried out experiments to find the best features to be used for classification. We use all possible combinations of these features to build the PNN classifier: RIRs, Fractal Dimension (FDs) and Hjorth parameters (Hjorth's). The performance of each PNN with a specific combination of features is tested using LOOCV against each channel. The results are listed in Table I where each entry is the accuracy of LOOCV of the PNN with the features for that column against the data set of the channel corresponding to that row.

From Table I, it is clear that the first feature combination (using all features) yields the highest accuracy, and thus we decide to use all extracted features in later experiments to build the classifiers.

The accuracy of the combined classifiers increases to 84.27% while the true and false positive rates increase to 85.36% and 83.18% respectively. Thus, the sensitivity and specificity are 83.33% and 84.69%, respectively.

B. Optimizing feature extraction parameters

In Sec. II and Sec. III, there are some parameters that can be changed: the segment length of EEG signal, the cut-off frequency of filters, and the bin (f_{step}) and band (f_{low} and f_{up}) in Eq. (1). A combination of those parameters is called a *configuration*. In this subsection, we will show that such configuration is important to the classification. Optimized configuration can lead to better accuracy. Different feature extraction parameters used in this paper are listed in Table II.

Table III shows accuracies of combined PNN based classifiers in different configurations. The cut-off frequency of 56 and 66 Hz are not tested for segment length 4096, because

TABLE II
FEATURE EXTRACTION PARAMETERS USED IN THIS PAPER

Parameters	Values
segment length	4096 or 8192 samples
cut-off frequency of filters	40, 46, 56 or 66 Hz
spectral band and bin	band: 2-32 Hz, bin: 1 Hz band: 2-34 Hz, bin: 2 Hz band: 2-34.5 Hz, bin: 2.5 Hz

TABLE III
ACCURACY OF VOTED CLASSIFIER (PNN) IN DIFFERENT CONFIGURATIONS

Length	cut-off freq.	band and bin ($f_{low}-f_{up}$, f_{step})			
		2-32, 1	2-34, 2	2-34.5, 2.5	
4096	40	86.41	84.27	83.41	
	46	91.77	89.81	89.23	
8192	40	90.19	87.80	86.86	
	46	93.73	91.93	91.92	
	56	94.07	92.14	91.37	
	66	93.78	91.96	91.13	

we find longer segmentation can give higher accuracy. An interesting finding is that after the filter cut-off frequency reaches 46Hz, the accuracy does not significantly increase. One possible explanation is that many spikes may exist in interictal EEG and most reside in a frequency range of 15 to 50 Hz. Increasing the filter cut-off frequency may also introduce line noise from power supply or other sources, which will not benefit EEG signal quality [27]. Table V shows the highest accuracy is 94.07%, which is almost the same as the reported epilepsy diagnosis accuracy by human in a medical journal [22].

VII. CONCLUSIONS

In this paper, an automated interictal scalp EEG recognition system for epilepsy diagnosis is developed and validated. Three classes of features are extracted and PNNs are employed to make classification using those features. To improve the accuracy, we optimize the feature extraction parameters and design a final classifier that combines several PNN-based classifiers. Our system can reach an accuracy of 94.07%, which is very close to the accuracy achieve by human. Compared with the existing approaches on epilepsy diagnosis, our approach does not require the occurrence of seizure activity during EEG recording. This merit reduces the difficulties in EEG collection since interictal data is much easier to be collected than ictal data. Therefore, our system is very helpful for areas short of medical resources.

REFERENCES

- [1] K. Lehnertz, F. Mormann, T. Kreuz, R. Andrzejak, C. Rieke, P. David, and C. Elger, "Seizure prediction by nonlinear EEG analysis," *IEEE Engineering in Medicine and Biology Magazine*, 2003.
- [2] *Atlas: Epilepsy Care in the World*. World Health Organization, 2005.
- [3] R. Flink, B. Pedersen, A. B. Guekht, K. Malmgren, R. Michelucci, B. Neville, F. Pinto, U. Stephani, and C. Ozkara, "Guidelines for the use of EEG methodology in the diagnosis of epilepsy international league against epilepsy," *Acta Neurologica Scandinavica*, vol. 106, 2002.
- [4] C. Logar, B. Walzl, and H. Lechner, "Role of long-term EEG monitoring in diagnosis and treatment of epilepsy," *European Neurology*, vol. 34, 1994.

- [5] T. S. Walczak, P. Jayakar, and E. M. Mizrahi, *Epilepsy: A Comprehensive Textbook*, 2nd ed. Lippincott Williams & Wilkins, 2008, ch. 73, pp. 809 – 813.
- [6] C. Bigan, “A recursive time-frequency processing method for neural networks recognition of EEG seizures,” in *Neural Networks and Expert Systems in Medicine and Healthcare*, E. C. Ifeachor, A. Sperduti, and A. Starita, Eds. Singapore: World Scientific, 1998, pp. 67–73.
- [7] A. Gardner, A. Krieger, G. Vachtsevanos, and B. Litt, “One-class novelty detection for seizure analysis from intracranial EEG,” *Journal of Machine Learning Research*, vol. 7, 2006.
- [8] V. Srinivasan, C. Eswaran, and N. Sriraam, “Artificial neural network based epileptic detection using time-domain and frequency-domain features,” *J. Med. Syst.*, vol. 29, no. 6, pp. 647–660, 2005.
- [9] W. Weng and K. Khorasani, “An adaptive structure neural networks with application to eeg automatic seizure detection,” *Neural Network*, vol. 9, no. 7, pp. 1223–1240, 1996.
- [10] M. K. Kiymik, A. Subasi, and H. R. Ozcalik, “Neural networks with periodogram and autoregressive spectral analysis methods in detection of epileptic seizure,” *J. Med. Syst.*, vol. 28, no. 6, pp. 511–522, 2004.
- [11] V. P. Nigam and D. Graupe, “A neural-network-based detection of epilepsy,” *Neurological Research*, vol. 26, pp. 55–60(6), 1 January 2004.
- [12] N. Pradhan, P. K. Sadasivana, and G. R. Arunodaya, “Detection of seizure activity in EEG by an artificial neural network: A preliminary study,” *Computers and Biomedical Research*, vol. 29, no. 4, pp. 303–313, 2002.
- [13] V. Srinivasan, C. Eswaran, and N. Sriraam, “Approximate entropy-based epileptic EEG detection using artificial neural networks,” *IEEE Transactions on Information Technology in Biomedicine*, vol. 11, no. 3, pp. 288–295, May 2007.
- [14] A. B. Geva and D. H. Kerem, “Forecasting generalized epileptic seizures from the EEG signal by wavelet analysis and dynamic unsupervised fuzzy clustering,” *IEEE Transactions on Biomedical Engineering*, vol. 45, pp. 1205–1216, 1998.
- [15] A. Alkan, E. Koklukaya, and A. Subasi, “Automatic seizure detection in EEG using logistic regression and artificial neural network,” *Journal of Neuroscience Methods*, vol. 148, no. 2, pp. 167 – 176, 2005.
- [16] N. McGorgan. (1999) Neural network detection of epileptic seizures in the electroencephalogram. [Online]. Available: <http://citeseer.ist.psu.edu/625725.html>
- [17] J. Gotman, “Automatic detection of seizures and spikes,” *J. Clin. Neurophysiol.*, vol. 16, pp. 130–140, 1999.
- [18] F. S. Bao, D. Y.-C. Lie, and Y. Zhang, “A new approach to automated epileptic diagnosis using eeg and probabilistic neural network,” *20th IEEE International Conference on Tools with Artificial Intelligence, 2008. ICTAI '08.*, vol. 2, pp. 482–486, Nov. 2008.
- [19] D. Specht, “Probabilistic neural networks,” *Neural Networks*, vol. 3, 1990.
- [20] C.-W. Ko and H.-W. Chung, “Automatic spike detection via an artificial neural network using raw eeg data: effects of data preparation and implications in the limitations of online recognition,” *Clinical Neurophysiology*, vol. 111, no. 3, pp. 477–481, March 2000.
- [21] R. O. Duda, P. E. Hart, and D. G. Stork, *Pattern Classification*, 2nd ed. John Wiley and Sons, 2001, ch. 9, pp. 471–486.
- [22] M. Salinsky, R. Kanter, and R. M. Dasheiff, “Effectiveness of multiple EEGs in supporting the diagnosis of epilepsy: an operation curve,” *Epilepsia*, vol. 28, pp. 331–334, 1987.
- [23] A. Petrosian, “Kolmogorov complexity of finite sequences and recognition of different preictal EEG patterns,” in *Proc. of the Eighth IEEE Symposium on Computer-Based Medical Systems*, 1995.
- [24] T. Higuchi, “Approach to an irregular time series on the basis of the fractal theory,” *Physica D*, vol. 31, no. 2, pp. 277 – 283, 1988.
- [25] B. Hjorth, “EEG analysis based on time domain properties,” *Electroencephalography and Clinical Neurophysiology*, vol. 29, pp. 306–310, 1970.
- [26] R. K. Orr, “Use of a Probabilistic Neural Network to Estimate the Risk of Mortality after Cardiac Surgery,” *Med. Decis. Making*, vol. 17, no. 2, pp. 178–185, 1997.
- [27] R. Aschenbrenner-Scheibe, T. Maiwald, M. Winterhalder, H. U. Voss, J. Timmer, and A. Schulze-Bonhage, “How well can epileptic seizures be predicted? An evaluation of a nonlinear method,” *Brain*, vol. 126, pp. 2616–2626, 2003.